
Hygro - Thermograph

1.0670.../ 1.0674.../ 1.0680...



ADOLF THIES GmbH & Co. KG

Hauptstraße 76

Box 3536 + 3541

Phone ++551 79001-0

www.thiesclima.com

37083 Göttingen Germany

37025 Göttingen

Fax ++551 79001-65

info@thiesclima.com

Contents

1	Models available	2
2	Application	3
3	Set-up and Mode of Operation.....	3
4	Preparation for Use.....	4
5	Maintenance	5
5.1	Changing the recording strip	5
5.2	Changing the recording pens	6
5.3	Regenerating the humidity measuring element.....	6
5.4	Checking the bimetallic setting.....	6
5.5	Static Charge.....	6
6	Technical Data.....	7
7	Scale Drawing.....	8

Tables

Table 1: models available.....	2
Table 2: Recording Strips.....	6

1 Models available

Order-No.	Recording Time	Clockwork
1.0670.xx.xxx	1 day / 7 days, switchable	Spring clockwork mechanism
1.0674.xx.xxx	14 days / 31 days, switchable	Spring clockwork mechanism
1.0680.xx.xxx	1 / 7 / 31 days, switchable	Quartz clockwork mechanism
Humidity measuring range		
...10...	H (10...100 % rel.h. ; -35...+80 °C)	
...12...	K (0...100 % rel.h. ; 0...+80 °C)	
Temperature measuring range		Graduation
...000	-35 ... +45 °C	1 °C
...005	-20 ... +60 °C	1 °C
...011	-10 ... +50 °C	1 °C
...014	0 ... +40 °C	0,5 °C
...017	0 ... +80 °C	1 °C

Table 1: models available

Attention:

■ *Hygro- Thermographs with Quartz clockwork mechanism are applicable only within a temperature range from –20 to +60°C!*

2 Application

The hygro-thermograph measures and records both the relative humidity and the air temperature of the surrounding atmosphere. The recording drum is driven with utmost precision either by a manual spring clockwork mechanism or by a battery-operated quartz clockwork. Either H or K humidity measuring elements can be used depending on the general on-site operating conditions.

"H" measuring elements are suitable for taking measurements in normal to very moist air at temperatures below and above 0°C.

"K" measuring elements are designed for use in normal to dry air in the temperature range above 0°C and require no maintenance.

Typical applications include environmental monitoring in computer rooms, factories, warehouses, offices, laboratories, nurseries, museums and galleries but they can also be used in meteorological measuring stations.

3 Set-up and Mode of Operation

The clockwork and the columns with the humidity measuring element and the temperature measuring element are mounted to a base plate. A transparent inverted cover made of UV-resistant polycarbonate is used for protection of the entire system. The measuring elements react promptly thanks to large ventilation openings in the direction of measurement.


Humidity is measured by a hair (H) or by a synthetic (K) measuring element. These measuring elements consist of several hairs or fibres whose lengths change when the humidity changes. This change in length is recorded by a felt pen onto a paper recording strip via a system of levers. The measurement accuracy indicated for the H measuring element applies to regenerated measuring elements in decreasing humidity.

Temperature is measured by a high quality, aged bimetallic measuring element which has been bent to form a ring. The radius of the measuring element changes when the temperature changes. This change in radius is likewise recorded on the recording strips. The rotation of the drum allows time-dependent registration.

4 Preparation for Use


For easy operation, the inverted drum of the quartz clockwork mechanism is simply set without any screws onto the central shaft. That is why the opened instrument may never be transported or carried on the inverted drum.

Unscrew the knurled screw, remove the inverted cover and remove the foam rubber (used for transport) from the clockwork. Press the switch-off lever to the right to raise the recording pens from the recording strip.

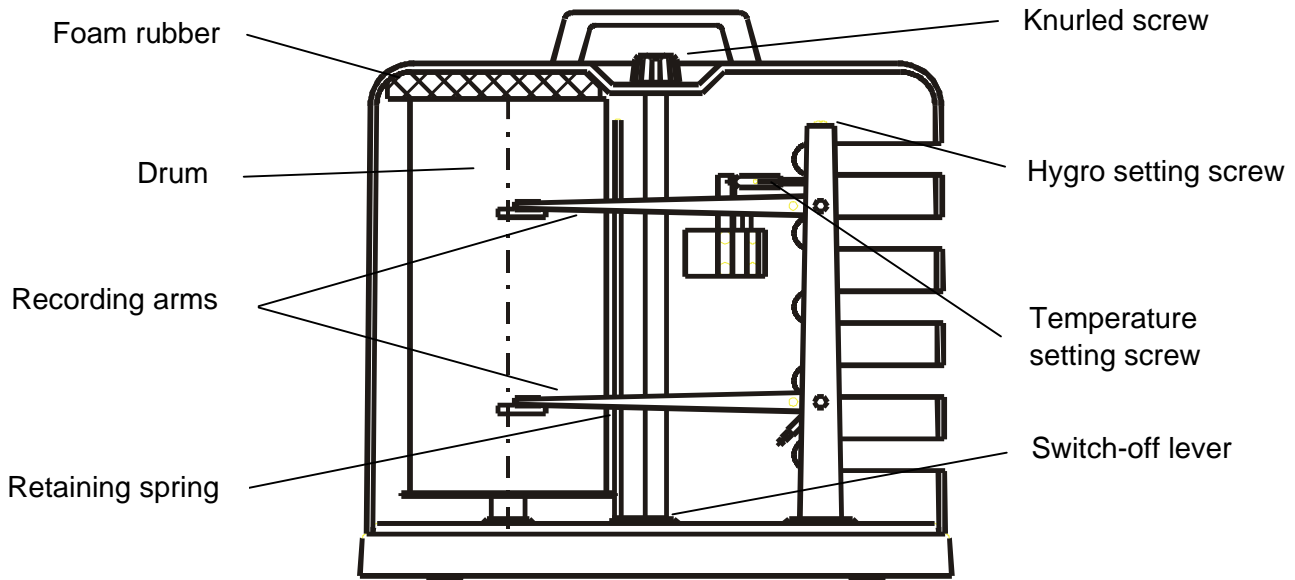

Setting the desired recording time

For instruments with a spring clockwork mechanism, unscrew the winding key by turning it towards the right and remove the inverted drum from the drive mechanism. The desired recording time can be set by changing the interchangeable gear wheel on the drum.

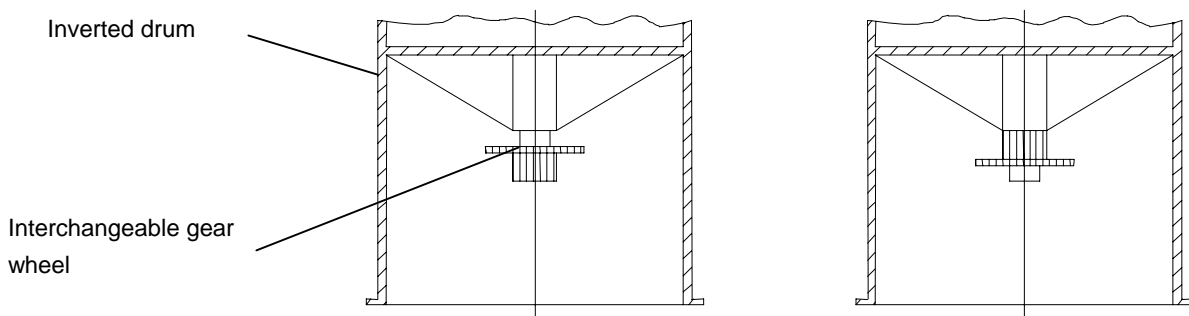


Order No.
1.0670.xx.xxx
1.0674.xx.xxx

Recording time
1 day
14 days

Recording time
7 days
31 days

Instrument with Quartz Clockwork:

Remove the inverted drum from the drive mechanism and set the recording time with the red gear wheel by clicking it into place at the appropriate height. Make sure that the yellow gear wheel is properly engaged. Place the enclosed battery into the recess provided with the poles in the correct direction.

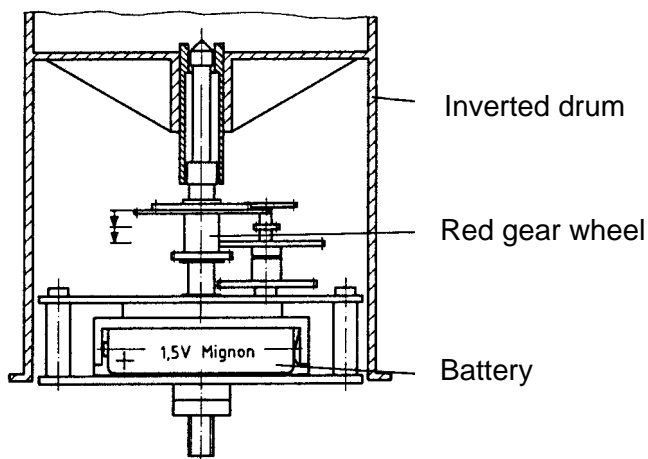

Position of the red gear wheel	
up	7 days
middle	31 days
down	1 day

Place the recording strip onto the inverted drum (see 6.1 Changing the recording strip) and insert this onto the drive mechanism until it locks into place!

Remove the lower recording arm from the clamp bolt (transport safety device). Remove the tip protector from the felt pen. For instruments with a spring clockwork mechanism, wind the clockwork with the key in the drum, turning it to the left. Rotate the drum counter clockwise to the correct time. Close the hood and screw the knurled-head screws back into place. Press the switch-off lever to the right stop in order to lower the recording pens onto the recording strip.

5 Maintenance

5.1 Changing the recording strip

This should be done regularly at the time where the recording strip starts; for example if you are using a 7 day recording period, then change the strip every Monday morning. After swinging the recording arm forwards, raise the chart holder and remove the recording strip. Place the new recording strip onto the drum and fix it into position by inserting the chart holder. Make sure that the new recording strip fits snugly and smoothly against the lower edge of the drum. Rewind the clockwork mechanism every time you change the recording strip. Swing the recording arms back to their original position and rotate the drum counter clockwise to the correct time. The instrument is now ready for use.

Recording Strips (1 set = 100 sheets), order-no. key

°C	"H" Measuring element				"K" measuring element			
	1 day	7 days	14 days	31 days	1 day	7 days	14 days	31 days
-35...+45	205142	205086	205153	205169				
-20...+60	205143	205083	205158	205168				
-10...+50	205138	205092	205155	205166				
0...+40	205123	205094	205150	205160	205131	205097	205151	205161
0...+80	205126	205103	205280	205281	205134	205112	205282	205283

Table 2: Recording Strips

5.2 Changing the recording pens

Remove the recording pens carefully from the recording arms. Remove the tip protection from the new pen. Make sure that you do not touch the recording tip when you place the new pen into position.

Spare Recording pens (minimum order of 6) Order-No. 500 847

5.3 Regenerating the humidity measuring element

"H" measuring elements dry out when the relative humidity is less than 60%. This results in an increase in the zero point of approximately 5% or more rel. humidity. At ca. 60% rel. humidity, maximum inaccuracy is reached in 3 weeks. This time is shorter when the humidity value is even lower. Accuracy can be restored by regeneration. Simply place the instrument in saturated air for some hours. At the conclusion of the regeneration process, check whether the measuring element has returned to 95% rel. humidity. This value can be set on the humidity setting screw.

Measuring elements which are located out-of-doors or in huts regenerate automatically because the central European climate is such that, particularly at night - humidities of 95% occur.

"K" measuring elements do not degenerate, and consequently do not have to be regenerated.

5.4 Checking the bimetallic setting

The accuracy of the bimetallic element is checked by carrying out a comparative measurement. In a temperature-constant room hang a precision mercury thermometer next to the hygro-thermograph. Allow about 20 minutes adjustment time and then compare the temperature values. If a correction is necessary, do this with the aid of the temperature setting screw on the bimetallic element.

5.5 Static Charge

A static charge arises when the cover is rubbed thoroughly with a cloth; then the recording arms stick on the cover side. In order to avoid to static charges it is recommended to clean the cover inside in regular intervals with the enclosed antistaticum.

6 Technical Data

Humidity

Measuring range	10 ... 100 % rel. humidity "H"
	0 ... 100 % rel. humidity "K"
Graduation	5 % rel. humidity
Temp.- working range	-35 ... +70°C "H"
	0 ... +80°C "K"
Measurement accuracy	± 2 % rel. humidity "H" + 1 Scale graduation @ 65% rel. h. and room temperature
	± 3 % rel. humidity "K" + 1 Scale graduation @ 65% rel. h. and room temperature

Temperature

Measuring range	-35 ... +80°C (see models available)
Graduation	1°C bzw. 0,5°C (see models available)
Measurement accuracy	± 1 % of measuring range + 1 Scale graduation

Clockwork

Spring clockwork mechanism	
Recording time	1 day / 7 days resp. 14 days / 31 days; (see models available)
Thrust	11,45 mm/h.; 40,01 mm/day resp. 20 mm/day; 9 mm/day
Temperature range	-35 ... +80°C
Gear accuracy	± 60 s/day at 20°C acc. to DIN 8300


Quartz clockwork

Recording time	1 day / 7 days / 31 days
Thrust	11.45 mm/h.; 40.01 mm/h; 9 mm/h
Temperature range	-20 ... +60°C similar to DIN 8300 B
Gear accuracy	± 2 s/day
Battery capacity	> 1 year at 20°C (mignon battery 1,5 V)

GENERALLY

Clockwork drum	S 93 x 186 similar to DIN 58658
Recording strip	Similar to DIN 16232
Recording width	2 x 82 mm
Weight	2.1 kg

7 Scale Drawing

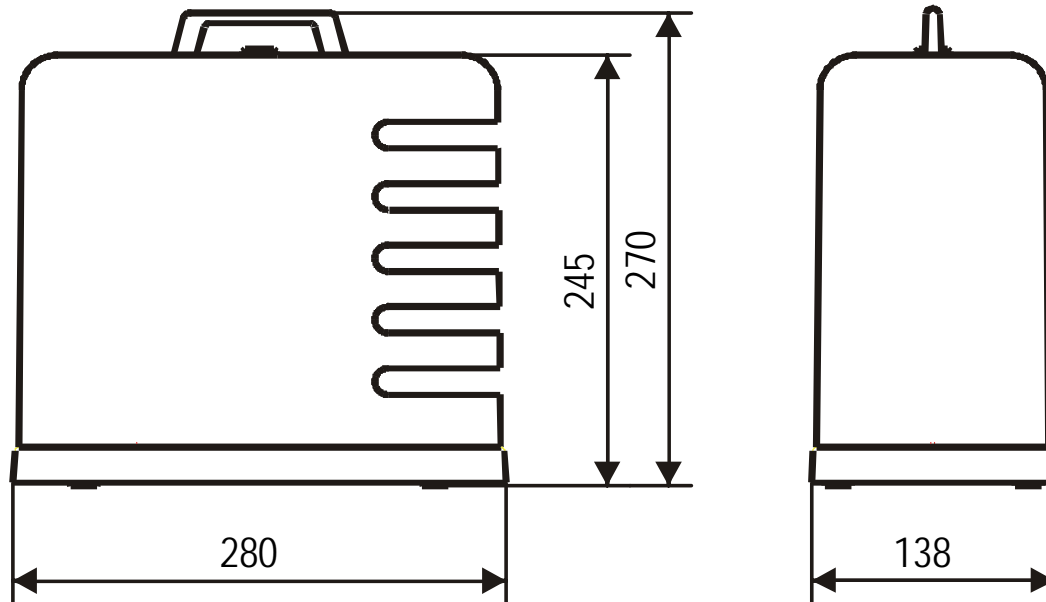

	ADOLF THIES GmbH & Co. KG		
	Hauptstraße 76 37083 Göttingen Germany P.O. Box 3536 + 3541 37025 Göttingen Phone ++551 79001-0 Fax ++551 79001-65 www.thiesclima.com info@thiesclima.com		

- Alterations reserved -